

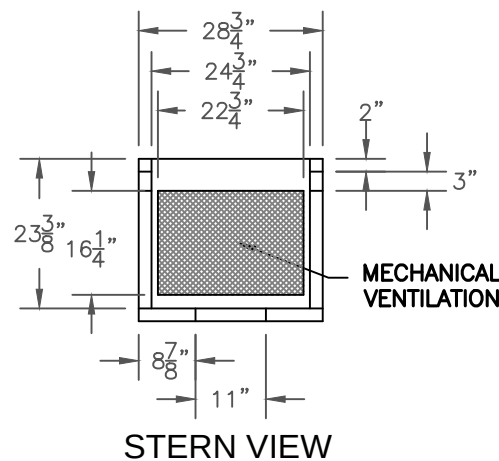


1 To maintain good air circulation for cooling, please maintain a minimum of 2" from the Stern, Starboard and Port sides to nearest wall.

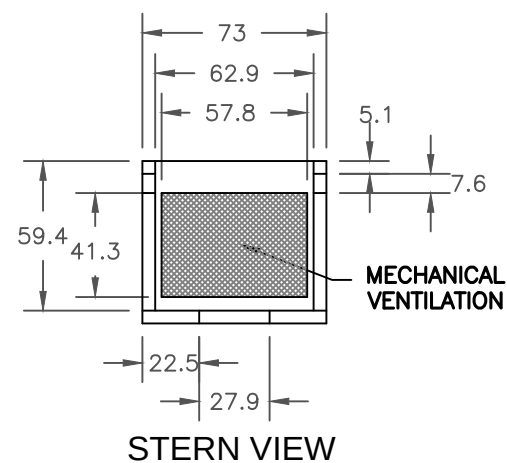

THE MOROZKO IS DESIGNED TO SUPPORT A HEALTHY LIFESTYLE, NOT DIAGNOSE, CURE, OR PREVENT SPECIFIC DISEASES OR MEDICAL CONDITIONS. MOROZKO ICE BATHS ARE NOT MEDICAL DEVICES, AND HAVE NOT BEEN EVALUATED BY THE FDA. MOROZKO MAKES NO CLAIMS OR WARRANTIES WITH REGARD TO THE HEALTH EFFECTS OF COLD PLUNGE THERAPY OR USE OF MOROZKO PRODUCTS. SEEK MEDICAL ADVICE FROM YOUR PHYSICIAN BEFORE EMBARKING ON A PROGRAM OF DELIBERATE COLD EXPOSURE.

1 To maintain good air circulation for cooling, please maintain a minimum of 50.8mm from the Stern, Starboard and Port sides to nearest wall.

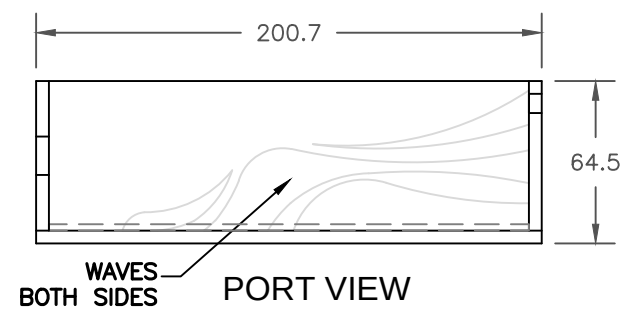

THE MOROZKO IS DESIGNED TO SUPPORT A HEALTHY LIFESTYLE, NOT DIAGNOSE, CURE, OR PREVENT SPECIFIC DISEASES OR MEDICAL CONDITIONS. MOROZKO ICE BATHS ARE NOT MEDICAL DEVICES, AND HAVE NOT BEEN EVALUATED BY THE FDA. MOROZKO MAKES NO CLAIMS OR WARRANTIES WITH REGARD TO THE HEALTH EFFECTS OF COLD PLUNGE THERAPY OR USE OF MOROZKO PRODUCTS. SEEK MEDICAL ADVICE FROM YOUR PHYSICIAN BEFORE EMBARKING ON A PROGRAM OF DELIBERATE COLD EXPOSURE.